



Establishing a Hospital-based I-125 Seed Breast Localization Program

Alan M. Daus, M.S., DABR
Diagnostic Physics Section
Gundersen Health Imaging Dept.

Need a pic of Grand Dads Bluff
looking over La Crosse

■ To

Objective

- To provide guidance on implementing a breast localization program using I-125

Disclaimer/Conflict of Interest

- We have just completed our 6th case.
- I have no conflict of interest in any vendor of I-125 seeds or any medical device used for this procedure.

Learning Objectives

- Understand the Radioactive Material (RAM) license requirements and the requirements of Authorized Users.
- Understand the merits of a I-125 seed breast localization or Radioactive Seed Localization (RDL) versus the standard wire localization procedure that is currently being used.
- Understand the necessary equipment needed and the limitations.

Learning Objectives (Cont.)

- Understand the level of RAM safety training needed based on personnel work locations.
- Understand the ramifications of a lost seed.

Topics

- What is it?
- Regulatory requirements
- Potential Hazards
- Equipment
- Seed tracking and handoff
- Training

I-125 Breast Seed Localization

This is a new procedure that involves a radiologist implanting a I-125 radioactive “seed” in a suspected cancer site. Days later the surgeon can use the gamma probe in a similar manner to a breast sentinel lymph node procedure to locate the seed(s)

I-125 (Iodine)

Low energy (27 keV)

Half-life 59.4 days




1-3 seeds implanted
in each patient





I-125 RSL Vs. Wire Localization (WL)

- RSL can be used in conjunction with Sentinel Node procedures that use Tc-99m sulfur colloid with a gamma probe with multiple window settings.
- Some Surgeons report that RSL produces fewer positive margins and reoperation rates than WL
- Some Surgeons report an improved surgical approach with RSL resulting in better cosmetic outcomes.


Implant Procedure

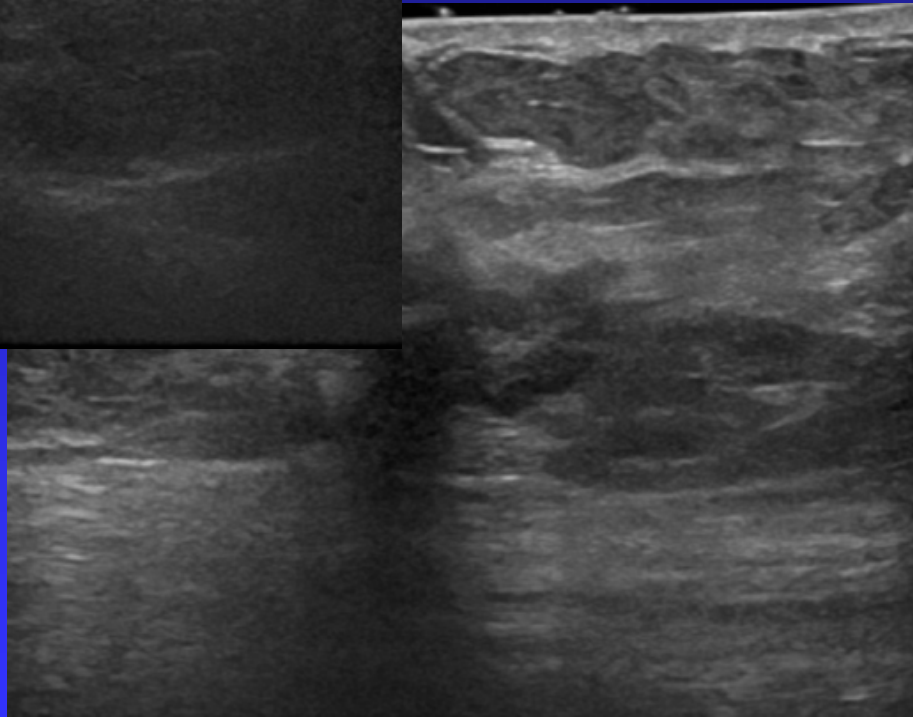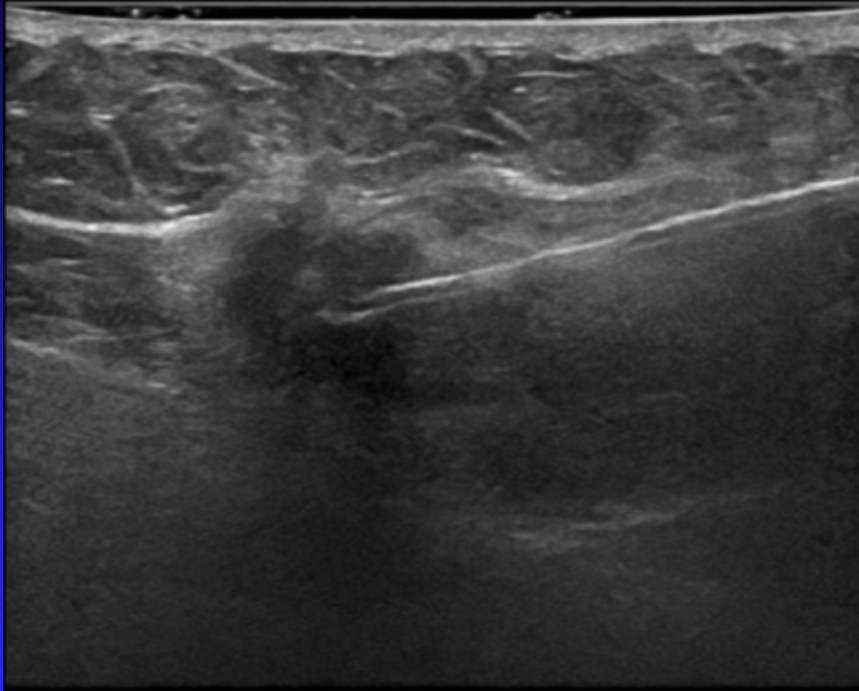



Verification of Implant

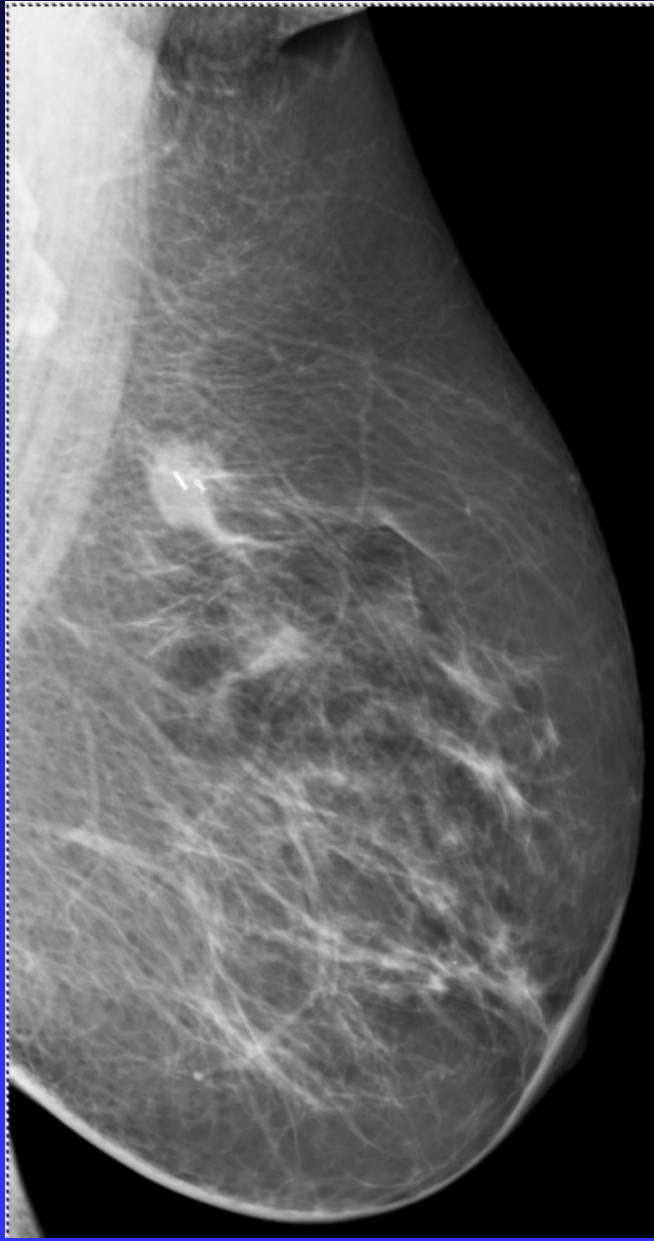

Results of Surgical Procedure

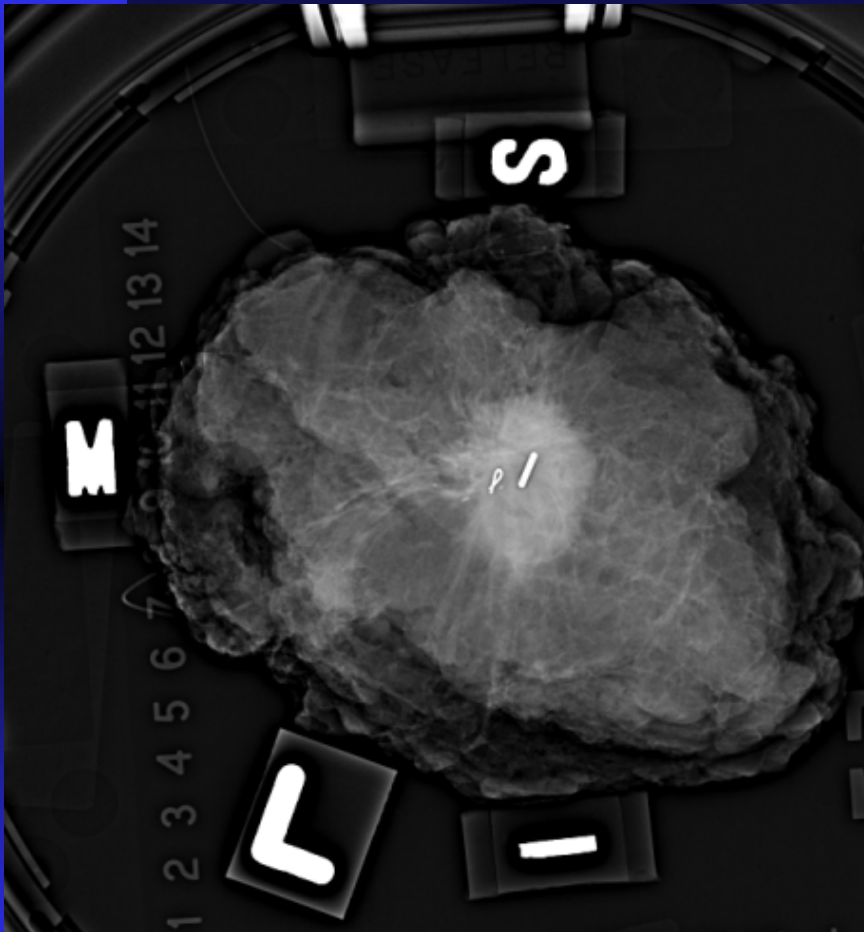

Histology Seed Extraction Procedure

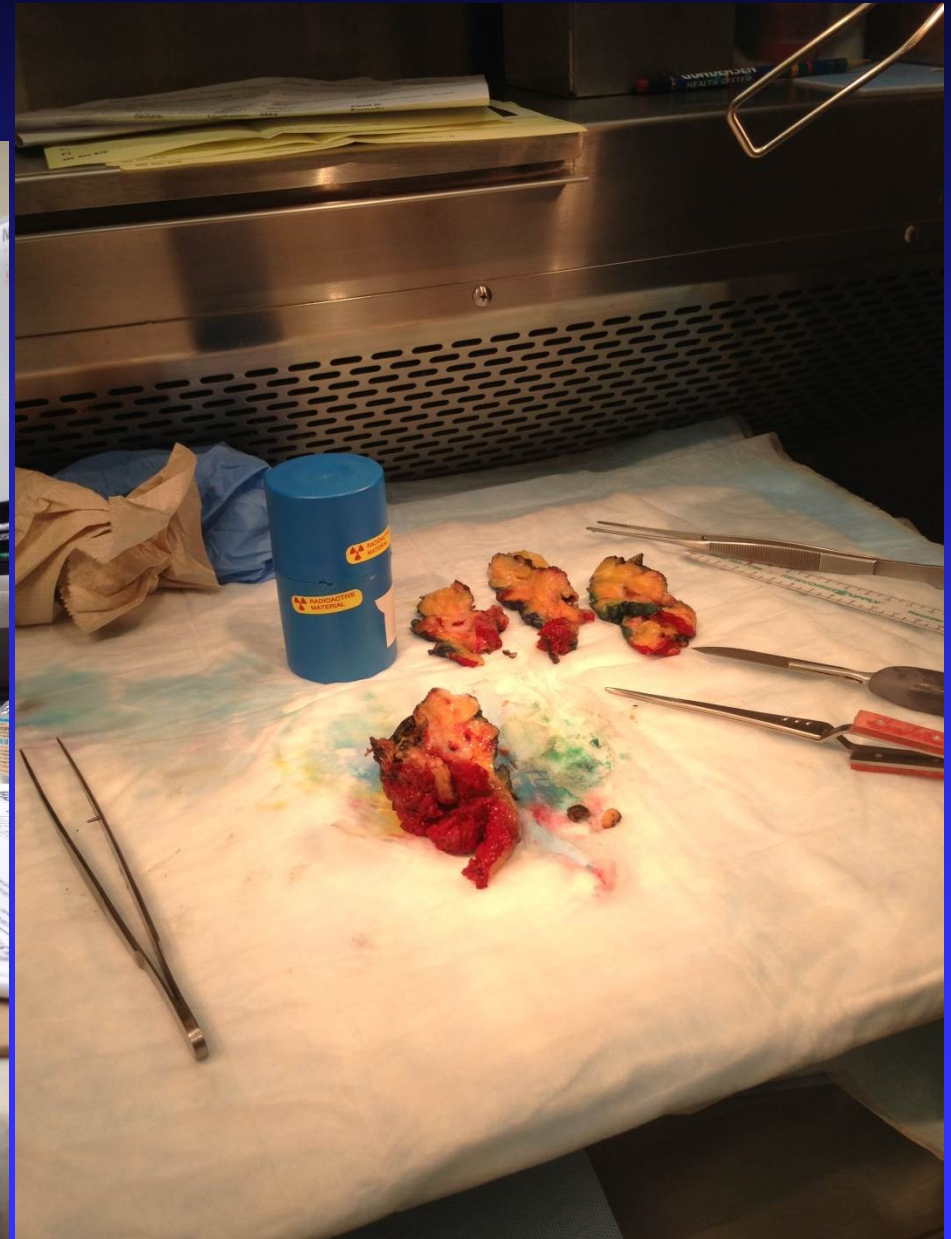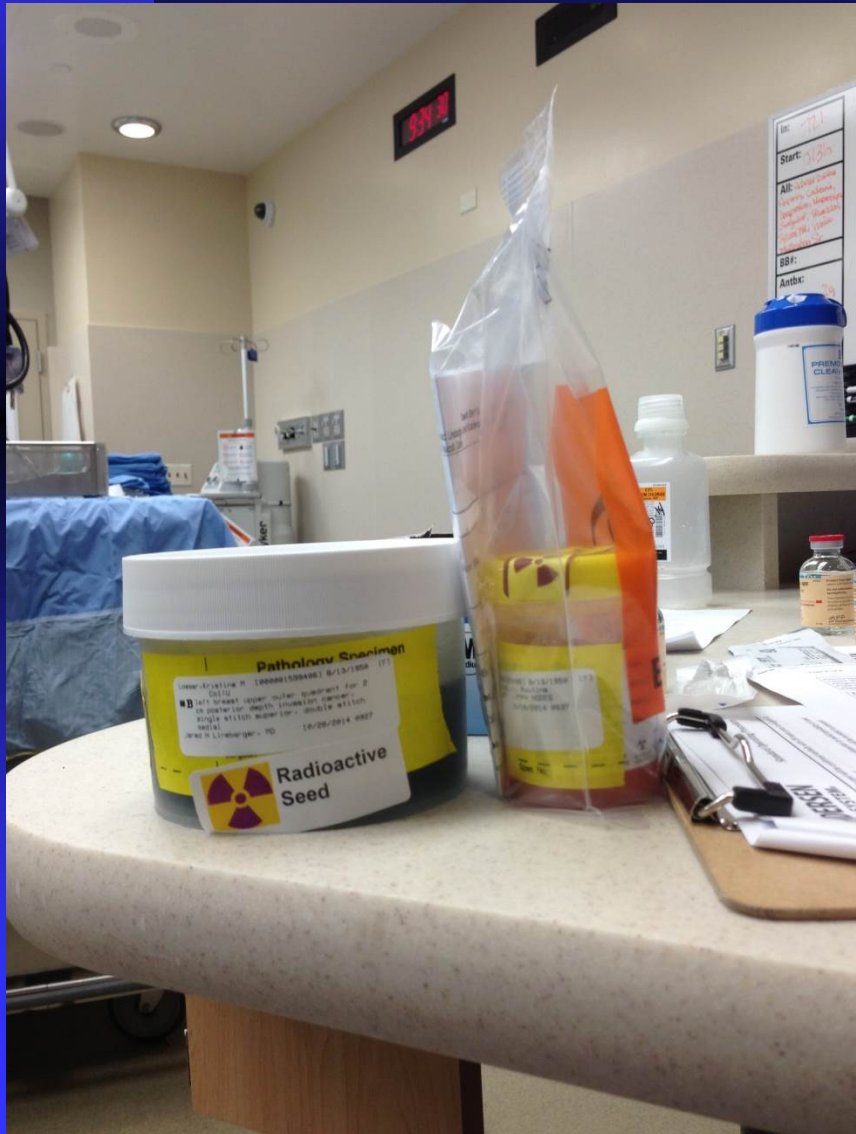

NRC and Agreement States Licensing Guidance

The use of these iodine-125 and palladium-103 seeds for therapy is currently regulated under 10 CFR 35.400: "Use of sources for manual brachytherapy" and the equivalent Agreement State regulations.

In the RSL procedure, the iodine-125 or palladium-103 seeds are implanted for localization by an authorized user and are not intended to deliver a therapeutic dose to tissue. Therefore, this application is not regulated under 10 CFR 35.400 or the equivalent Agreement State regulation.

The use of these seeds for RSL procedures will be regulated under 10 CFR 35.1000: "Other medical uses" and the equivalent Agreement State regulations.

NRC and Agreement States Licensing Guidance (cont.)

If the licensee intends to transfer the radioactive tissue samples, i.e., the tissues will still contain the seed(s), or more than 1 microcurie of iodine-125 or 100 microcuries of palladium-103 contamination from a leaking source, to an outside pathology laboratory, the licensee must ensure before shipment that the samples will be transferred to an NRC or Agreement State licensed laboratory authorized to receive the seeds or radioactive contaminated tissue (10 CFR 30.41). The applicant must also ensure that packages will be properly prepared in accordance with 10 CFR 71.5 or an equivalent Agreement State regulation for shipping.

NRC and Agreement States Licensing Guidance (cont.)

If the licensee intends to transfer the radioactive tissue samples, i.e., the tissues will still contain the seed(s), or more than 1 microcurie of iodine-125 or 100 microcuries of palladium-103 contamination from a leaking source, to an outside pathology laboratory, the licensee must ensure before shipment that the samples will be transferred to an NRC or Agreement State licensed laboratory authorized to receive the seeds or radioactive contaminated tissue (10 CFR 30.41). The applicant must also ensure that packages will be properly prepared in accordance with 10 CFR 71.5 or an equivalent Agreement State regulation for shipping.

Reporting

If a seed is lost, ruptured or if a patient doesn't return in a reasonable time one may have to report to the NRC or agreement state.

Talk about Danbury Incident. Express to patient the importance of returning for seed explant.

www.nrc.gov/materials/miau/med-use-toolkit/seed-localization.html


For example, if a patient doesn't return she can receive a dose of 70.2 cGy/MBq or 2.6 cGy/microCurie at 1 cm. Even a seed as small as 100 microCuries can result in 260 cGy from the time it is implanted to decay.



Radiation Safety Committee (RSC)

- If you have a RSC you will most likely need the committee approval in order to submit your amendment to the state.
- Discuss what will happen if a seed is lost. Talk about all the different fingers in the pie

Potential Hazards

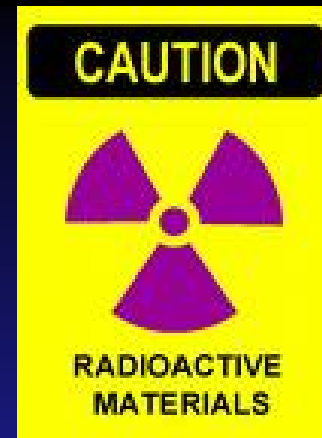

- Radiation exposure from seeds
- Handling. Radiation dose to hands can be high if seeds aren't handled safely. Safe at a distance.
- A broken seed can contaminate personnel, equipment, and the immediate area. I-125 can be taken up by thyroid tissue of the patient. Potassium Iodine (KI) (Lugal Solution) may have to be administered to the patient to act as a thyroid blocking agent.
- Lost seed(s) means a lockdown in the area until the seed(s) is found. Must check linen, containers, bottom of personnel shoe, etc. until seed is found. Lockdown means nothing enters or leaves the area until the seed is found.

The use of I-125 for RSL or breast seed localization is governed by what section of NRC or agreement state radioactive material license:

20%

1. Manual Brachytherapy

20%

2. Other Medical Use

20%

3. Uptake, Dilution and Excretion

20%

4. Imaging and Localization

20%

5. Diagnostic or Radiotherapy

The use of I-125 for RSL or breast seed localization is governed by what section of NRC or agreement state radioactive material license:

- 2. Other Medical Use

Reference: www.nrc.gov/materials/miau/med-use-toolkit/seed-localization.html

The Authorized User of I-125 for RSL or breast seed localization can be a physician performing:

- 20% 1. Uptake and dilution studies
- 20% 2. Imaging & localization studies
- 20% 3. High dose brachytherapy via afterloader
- 20% 4. Manual brachytherapy
- 20% 5. Radioactive drugs for medical use

The Authorized User of I-125 for RSL or breast seed localization can be a physician performing:

- 4 Manual brachytherapy

Reference: www.nrc.gov/materials/miau/med-use-toolkit/seed-localization.html

If your facility is planning on transferring breast specimens containing I-125 radioactive seeds to an outside laboratory then you must follow proper DOT shipping procedures and ensure that the lab:

- 20% 1. Disposes of the seed right after the seed is removed
- 20% 2. Is Accredited
- 20% 3. Has a NRC or Agreement State RAM License
- 20% 4. Has enough personnel
- 20% 5. Is located nearby

If your facility is planning on transferring breast specimens containing I-125 radioactive seeds to an outside laboratory then you must follow proper DOT shipping procedures and ensure that the lab:

3. Has a NRC or Agreement State RAM License

Reference: www.nrc.gov/materials/miau/med-use-toolkit/seed-localization.html

Emergency Kit



In all three locations (CBC , Surgery and Pathology) an emergency kit will be present in the room any time a seed is implanted or removed. The kit is there because if a seed is lost or damaged one can't leave the immediate area. The emergency kit will contain

1. Survey meter with thin window NaI probe.
2. A shielded container for the seed
3. Reverse pressure forceps



Emergency Kit – with Instructions



Other Equipment Considerations

You may find that your surgery/OR doesn't want to give up any of the gamma probes that are used for sentinel node procedures. This is a problem since Pathology/Histology will be the ones digging the seed(s) out of the specimen. We found a refurbished gamma probe unit that permanent resides in histology

Seed Tracking & Inventory

Seed Received by Radiation Oncology					Breast Center Seed Inventory							
Date Arrived	Number	Activity per seed	Total Activity	Initials	Date Received	Initials	Action	Seeds Received from	# Seeds Received	# Unused Seeds in CBC	# Used Seeds DIS	Total Inventory
11/5/13	5	0.11	0.55	JW	11/5/13	SAS	Locked in cupboard	Rad/Onc	5	5	0	5
					11/11/13	SAS	Locked in cupboard	Pathology	1	4	1	5

Seed Tracking & Inventory

RADIOACTIVE SEED LOCALIZATION (RSL) WRITTEN DIRECTIVE

Patient Name: _____
Clinic ID: _____
Diagnosis: _____
Date Scheduled for Implant: _____
Date Scheduled for Explant: _____

Center for Breast Care

Date of Implant: _____ Radioisotope: Iodine-125
Treatment site: _____
Number of seeds implanted: _____
Additional treatment site (if needed) _____
Number of seeds implanted: _____
Seed activity: _____ milliCurie
Total source strength (total number of seeds x seed activity): _____ milliCurie

Authorized User's signature: _____ *Date:* _____

Skin site/s marked "SEED": Y N
Seed armband placed on patient: Y N
Radiation survey of procedure room: _____ mR/hr (must be <0.04 mR/hr)

Seed Tracking & Inventory (cont.)

Surgery/OR

Date of explant: _____

Surgeon/Surgical Resident confirm "SEED" marking and wristband: Y N

Surgeon reviews Written Directive prior to explant: Y N

Number of Seeds removed: _____

Number of seeds on specimen image matches number of seeds implanted: Y N

Surgeon's signature: _____ *Date:* _____

Specimen delivered to Pathology/Lab by _____(name) at _____(time)

Specimen delivered to: _____(name)

Pathology

Specimens entered in log book by: _____(name) on _____(date)

Date Seeds Removed from specimen: _____

Name of Pathologist/Pathology Assistant removing seeds: _____

Number of Seeds removed: _____

Number of Seeds removed matches number of seeds from radiologist/surgeon: Y N

Seeds placed in vial and vial labeled with patient ID: Y N

CBC notified by _____(name) at _____(time) that seeds are ready for pickup

Seed Tracking & Inventory (cont.)

Center for Breast Care

Seeds retrieved from Pathology by: _____ (name) on _____ (date)

Number of seeds retrieved: _____

Number of Seeds removed matches number of seeds from radiologist/surgeon Y N

Seeds logged into storage in CBC Y N

Diagnostic Physics

Date of disposal: _____

Disposed by: _____ (name)

Disposal method: _____

Number of seeds disposed: _____

Number of seeds disposed matches number of seeds from radiologist/surgeon Y N

Survey meter ID: _____ Background: _____ mR/hr

Measured exposure rate: _____ mR/hr

The best equipment to assist in locating a lost I-125 seed is:

- 20% 1. Ionization Chamber
- 20% 2. GM survey meter with Beta probe
- 20% 3. GM survey meter with NaI probe
- 20% 4. Equipment used to test x-ray devices
- 20% 5. Photometer

The best equipment to assist in locating a lost I-125 seed is:

- 3 GM survey meter with NaI probe

Reference: www.nrc.gov/materials/miau/med-use-toolkit/seed-localization.html

Training Staff

- Breast Radiologists and Mammographers
- Breast Surgeons and OR Staff
- Pathology or Histology

ALARA and Radioactive Seeds

Use Distance! Step back when possible.

Although the exposure rate to personnel from unshielded radioactive seeds is very high at their surface, it drops to background level at 1 meter

Once the seeds are implanted the exposure rate drops to background level at 18-24 inches (due to shielding from tissue)

ALARA and Radioactive Seeds

Use Shielding! Keep seeds in a shielded container except when being used. When seeds are in incised tissue then the tissue sample should be placed in a shielded container

If you have to pick up a loose seed, use the reverse pressure forceps from the seed tray and put the seed in a shielded container.

Pre & Post-Procedure



All seeds must be accounted for in CBC when the seed(s) are implanted, when the incised tissue is removed in surgery and when the seeds are removed from the tissue in Lab.

In CBC, a mammogram will be done to ensure all seed implanted are physically located in the tissue.

In surgery a specimen radiograph will be made to verify the correct number of seeds are in the excised tissue and the remaining tissue will be surveyed to ensure no seed ruptured or was severed in two during the procedure. Depending on the view of the radiography it can be difficult to see a complete seed .

Pre & Post-Procedure (Cont.)



In the pathology lab, a physical count will be made and compared to the surgery/radiologists notes for the correct number of seeds.

At no time are scissors to be used to remove the seed from tissue. Scalpels and tweezers/reverse pressure forceps are the only items to be used

Pre & Post-Procedure (Cont.)



In all three locations (CBC, Surgery and Pathology) when the # of seed(s) is/are verified one must still use the radiation survey meter in the area to verify that no seeds are present. Lab personnel will contact CBC personnel to pick up seeds

To ensure that no seeds are lost, all waste material, waste containers, instrument trays, and linens must be surveyed with a radiation survey meter after the procedure and documented.

Source Security



- State law requires radioactive material to be under the licensee's control at all times.
- All radioactive seeds must be with an authorized individual or in a locked location at all times.

Source Security - Sterilization

- Seeds are obtained in pre-loaded, sterilized needles.

Why does one have to use a radiation survey meter or gamma probe to ensure all seeds have been removed if the seed can be seen in a breast specimen radiograph :

- 20% 1. The seed is not radiographic
- 20% 2. The seed could have multiplied
- 20% 3. The seed could have become more radioactive
- 20% 4. The seed could have been transected
- 20% 5. The seed could have moved

Why does one have to use a radiation survey meter or gamma probe to ensure all seeds have been removed if the seed can be seen in a breast specimen radiograph :

- 4. The seed could have been transected
- Radioactive Seed Localization with I-125 Non-Palpable Lesion Prior to Breast Lumpectomy and/or Excisional Biopsy: Methodology, Safety, and Experience of Initial Year, Dauer et al., Health Physics 105(4):356-365; 2013

Dosimetry Badges



- At this time we are not planning on monitoring radioactive seed implant staff at GL for occupational radiation dose. We may monitor pathology

References

- NUREG-1556, Volume 9, U.S. Nuclear Regulatory Commission, October 2002.
- www.nrc.gov/materials/miau/med-use-toolkit/seed-localization.html
- “Radioactive Seed Localization with I-125 Non-Palpable Lesion Prior to Breast Lumpectomy and/or Excisional Biopsy: Methodology, Safety, and Experience of Initial Year, Dauer et al., Health Physics 105(4):356-365; 2013

Acknowledgements

- Mary Ellen Jafari – Colleague for pictures and writing the RAM amendment
- Breast Radiologists at Gundersen Health System

Questions?