


Small Field Dosimetry: Overview of AAPM TG-155 and the IAEA-AAPM Code of Practice (Therapy)

Indra J. Das, PhD, FAAPM, FACR, FASTRO
Department of Radiation Oncology
Indiana University School of Medicine
Indianapolis, Indiana, USA

Small Field Dosimetry Problem

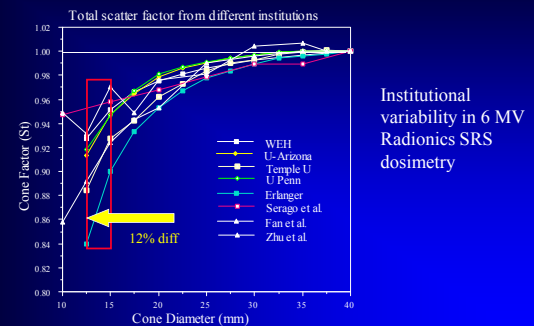


IJDas (2)

Das et al, J Radiosurgery, 3, 177-186, 2000



Dosimetric Variation with Detectors

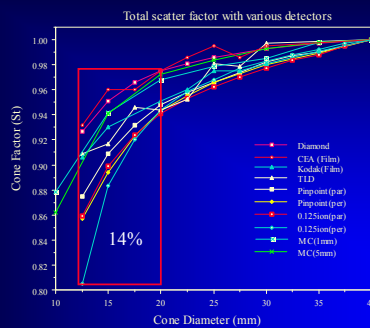

IJDas (3)

Das et al, J Radiosurgery, 3, 177-186, 2000




What is a Small Field?

- ❖ Lack of charged particle
 - ★ Dependent on the range of secondary electrons
 - ★ Photon energy
- ❖ Collimator setting that obstructs the source size
- ❖ Detector is comparable to the field size

IJDas (4)



Definition of Small Fields

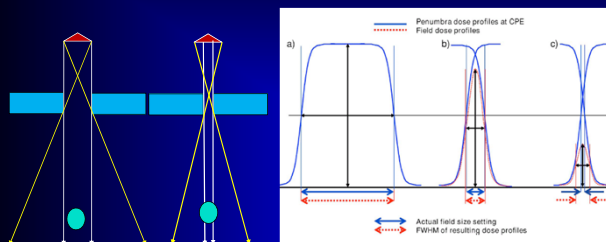


IJDas (5)

Das et al, Med. Phys. 35, 206-215, 2008



Energy Fluence Penumbra/Output

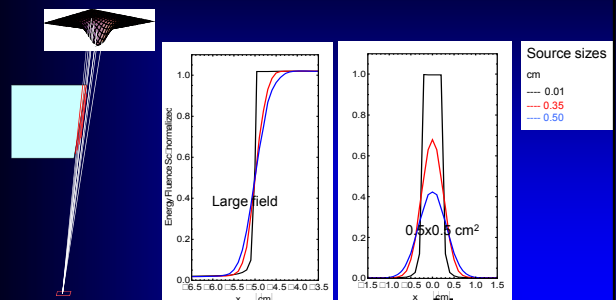


IJDas (6)

Nyhlm et al Radiother Oncol 78, 347, 2006 and Phys Med Biol 51,6245, 2006



Source Size

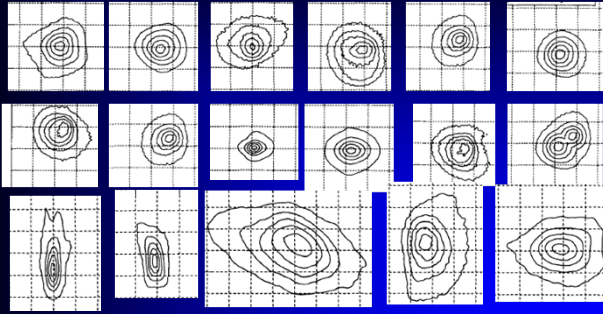

90%, 70%, 50%, 30%, 10% iso-intensity line
Jaffray et al, Med Phys 20, 1417-1427 (1993)

IJDas (7)



Source Size, Modern Machines

Varian TrueBeam


	T1	T2	T3	Dimensions x, y (mm)
6 MV				0.9, 0.7
6 MV FFF				0.8, 0.7
10 MV				0.9, 0.9
10 MV FFF				0.9, 0.8

IJDas (8)

Sawkey et al, Med Phys, 40, 332, 2013



IAEA/AAPM Proposed Pathway

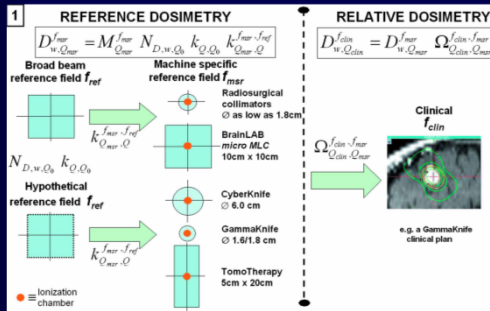

Alfonso, et al. Med Phys 35, 5179-5186 (2008)

IJDas (9)



Why So Much of Fuss?

- ❖ Reference (ref) conditions cannot be achieved for most SRS devices (cyberknife, gammaknife, tomotherapy etc)
- ❖ Machine Specific reference (msr) needs to be linked to ref
- ❖ Ratio of reading (PDD, TMR, Output etc) is not the same as ratio of dose

$$\frac{D_1}{D_2} \neq \frac{M_1}{M_2}$$

$$\frac{D_1}{D_2} = \frac{M_1}{M_2} \cdot \left[k_{Q_{clin}, Q_{msr}}^{f_{clin}, f_{msr}} \right]$$

IJDas (10)



Relative Dosimetry

$$D_{w, Q_{msr}}^{f_{msr}} = M_{Q_{msr}}^{f_{msr}} N_{D, w, Q_0} k_{Q, Q_0} k_{Q_{msr}, Q}^{f_{msr}, f_{ref}}$$

$$\Omega_{Q_{clin}, Q_{msr}}^{f_{clin}, f_{msr}} = \frac{M_{Q_{clin}}^{f_{clin}} \left(\frac{D_{w, Q_{clin}}^{f_{clin}}}{(M_{Q_{clin}}^{f_{clin}})} \right)}{M_{Q_{msr}}^{f_{msr}} \left(\frac{D_{w, Q_{msr}}^{f_{msr}}}{(M_{Q_{msr}}^{f_{msr}})} \right)} = \frac{M_{Q_{clin}}^{f_{clin}}}{M_{Q_{msr}}^{f_{msr}}} k_{Q_{clin}, Q_{msr}}^{f_{clin}, f_{msr}}$$

$$k_{Q_{clin}, Q_{msr}}^{f_{clin}, f_{msr}} = \frac{(D_{w, Q_{clin}}^{f_{clin}}) / (M_{Q_{clin}}^{f_{clin}})}{(D_{w, Q_{msr}}^{f_{msr}}) / (M_{Q_{msr}}^{f_{msr}})} = \frac{(Output)_{rel}}{(Reading)_{rel}}$$

$$k_{Q_{clin}, Q_{msr}}^{f_{clin}, f_{msr}} = \frac{(S_{w, air})_{f_{clin}} \cdot P_{f_{clin}}}{(S_{w, air})_{f_{msr}} \cdot P_{f_{msr}}}$$

IJDas (11)




Meaning of k in Micro-Chambers

$$k_{Q_{clin}, Q_{msr}}^{f_{clin}, f_{msr}} = \frac{\left[\left(\frac{\bar{L}}{\rho} \right)_{air}^w \cdot P_{fl} \cdot P_{grad} \cdot P_{stem} \cdot P_{cell} \cdot P_{wall} \right]_{f_{clin}}}{\left[\left(\frac{\bar{L}}{\rho} \right)_{air}^w \cdot P_{fl} \cdot P_{grad} \cdot P_{stem} \cdot P_{cell} \cdot P_{wall} \right]_{f_{msr}}}$$

IJDas (12)



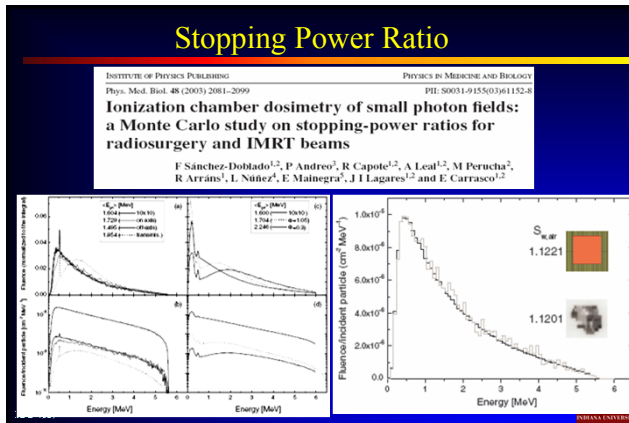


Radiological Parameters

Beam quality (TPR _{20,10})	$R_{w,air}$		$R_{PDA,air}$		Configuration
	Andreo (1994) ^a	This work	Andreo (1994) ^a	This work	
Elekta SL-18 radiosurgery					
10 × 10 cm ²	0.690	1.1187	1.1188	1.000	figure 1(a)
1.0 cm diameter			1.1155	0.997	figure 1(b)
0.3 cm diameter			1.1153	0.997	figure 1(c)
Siemens Primus MLC					
10 × 10 cm ²	0.677	1.1213	1.1221	1.001	figure 1(d)
2 × 2 cm ² irregular on-axis			1.1203	0.999	figure 1(e)
2 × 2 cm ² irregular 8 cm off-axis			1.1250	1.003	figure 1(f)
MLC transmission			1.1300	1.008	figure 1(i)
IMRT beam (10 × 10 cm ² approx)			1.1201	0.999	figure 12

^a These are the values in the IAEA TRS-398 code of practice (Andreo et al 2000).

Sánchez-Doblado et al, *Phys. Med. Biol.*, 48, 2081, 2003

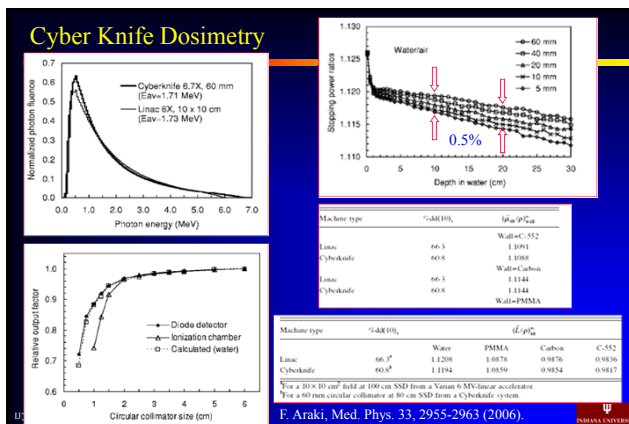


Correction Factors

Correction Factor depends on:

- Field size
- Source size (FWHM)
- Detector type

TABLE VII. F_{cor} of the four detectors for the 5, 7.5, and 10 mm collimators, as a function of the FWHM.				
FWHM (mm)	5 mm coll	7.5 mm coll	10 mm coll	
1.4	1.067	1.021	1.008	
1.8	1.087	1.017	1.007	
2.2	1.102	1.020	1.012	
2.6	1.112	1.027	1.010	
Pin Point				
FWHM (mm)	5 mm coll	7.5 mm coll	10 mm coll	
1.4	1.082	1.025	1.017	
1.8	1.099	1.024	1.013	
2.2	1.110	1.025	1.013	
2.6	1.124	1.037	1.016	
Diode				
FWHM (mm)	5 mm coll	7.5 mm coll	10 mm coll	
1.4	0.953	0.966	0.978	
1.8	0.955	0.966	0.978	
2.2	0.957	0.967	0.978	
2.6	0.940	0.967	0.978	
Diamond				
FWHM (mm)	5 mm coll	7.5 mm coll	10 mm coll	
1.4	1.066	1.001	1.001	
1.8	1.093	1.007	1.000	
2.2	1.107	1.010	0.999	
2.6	1.123	1.012	1.001	

Francescon, et al *Med Phys* 35, 504, 2008

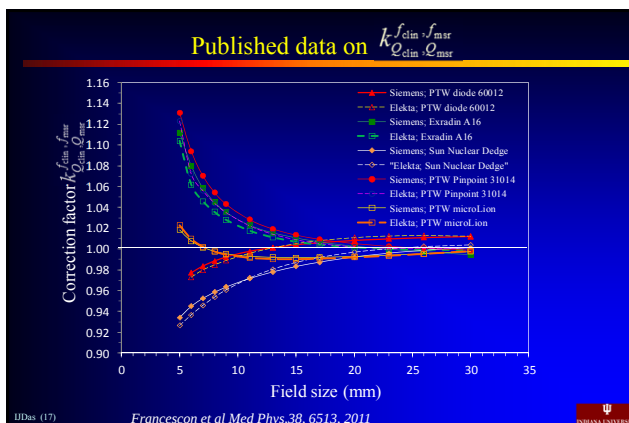

$k_{Q,lin}^{f_{lin}} / k_{Q,lin}^{f_{msr}}$ of Linear Accelerators (Varian)

Implementing a newly proposed Monte Carlo based small field dosimetry formalism for a comprehensive set of diode detectors

G. Crammer-Sargison¹⁾
Department of Medical Physics, Saskatchewan Cancer Agency, Saskatoon, Saskatchewan S7N 4H4, Canada
and Division of Medical Physics, Leeds Institute of Genetics, Health and Therapeutics, University of Leeds, Leeds LS2 9JT, United Kingdom

S. Weston
Department of Medical Physics and Engineering, St James's University Hospital, Leeds LS9 7TF, United Kingdom

J. A. Evans
Division of Medical Physics, Leeds Institute of Genetics, Health and Therapeutics, University of Leeds, Leeds LS2 9JT, United Kingdom

N. P. Sidhu
Saskatoon Cancer Centre, Saskatchewan Cancer Agency, Saskatoon, Saskatchewan S7N 4H4, Canada
and Department of Physics and Engineering, University of Saskatchewan, Saskatoon, Saskatchewan S7N 5E2, Canada

D. I. Thwaites
Institute of Medical Physics, School of Physics, University of Sydney, Sydney NSW 2006, Australia
and Division of Medical Physics, Leeds Institute of Genetics, Health and Therapeutics, University of Leeds, Leeds LS2 9JT, United Kingdom

(Received 21 April 2011; revised 11 October 2011; accepted for publication 14 October 2011; published 23 November 2011)

Med. Phys. 38 (12), 6992, 2011

$k_{Q_{\text{clin}} \rightarrow Q_{\text{msr}}}^{f_{\text{clin}} \rightarrow f_{\text{msr}}}$ of Linear Accelerators

Calculation of $k_{Q_{\text{clin}} \rightarrow Q_{\text{msr}}}^{f_{\text{clin}} \rightarrow f_{\text{msr}}}$ for several small detectors and for two linear accelerators using Monte Carlo simulations

P. Francescon,^{a)} S. Cora, and N. Satariano
Department of Medical Physics, ULSS 6–36100 Vicenza, Italy

Med. Phys. 38 (12), 6513-6527, 2011

Contents lists available at ScienceDirect
Radiotherapy and Oncology
journal homepage: www.thegreenjournal.com

Experimental small field 6 MV output ratio analysis for various diode detector and accelerator combinations

Gavin Crammer-Sargison^{a,b,c}, Steve Weston^{b,c}, Narinder P. Sidhu^{a,d}, David I. Thwaites^{b,e}

Radiotherapy and Oncology 100 (2011) 429–435





UDas (19)

$k_{Q_{\text{clin}} \rightarrow Q_{\text{msr}}}^{f_{\text{clin}} \rightarrow f_{\text{msr}}}$ Cyber Knife

Detector	5 mm		7.5 mm		10 mm	
	$M_{Q_{\text{clin}}}^{f_{\text{clin}}} / M_{Q_{\text{msr}}}^{f_{\text{msr}}}$	$k_{Q_{\text{clin}} \rightarrow Q_{\text{msr}}}^{f_{\text{clin}} \rightarrow f_{\text{msr}}}$	$M_{Q_{\text{clin}}}^{f_{\text{clin}}} / M_{Q_{\text{msr}}}^{f_{\text{msr}}}$	$k_{Q_{\text{clin}} \rightarrow Q_{\text{msr}}}^{f_{\text{clin}} \rightarrow f_{\text{msr}}}$	$M_{Q_{\text{clin}}}^{f_{\text{clin}}} / M_{Q_{\text{msr}}}^{f_{\text{msr}}}$	$k_{Q_{\text{clin}} \rightarrow Q_{\text{msr}}}^{f_{\text{clin}} \rightarrow f_{\text{msr}}}$
A16	0.626 (15)	1.089 (3)	0.811 (10)	1.018 (3)	0.866 (6)	1.010 (3)
PinPoint	0.620 (17)	1.101 (3)	0.801 (7)	1.024 (3)	0.862 (5)	1.015 (3)
Diode 60008	0.726 (1)	0.943 (3)	0.873 (1)	0.949 (3)	0.912 (1)	0.964 (3)
Diode 60012	0.705 (1)	0.956 (3)	0.847 (2)	0.966 (3)	0.891 (1)	0.978 (3)
EDGE	0.726 (1)	0.948 (3)	0.864 (1)	0.955 (3)	0.906 (1)	0.966 (3)
Alanine	0.544 (8)	1.249 (8)	0.785 (12)	1.059 (4)	0.855 (13)	1.019 (3)
TLD	0.668 (4)	...	0.809 (6)	...	0.880 (8)	...
EBT films	0.659 (17)	...	0.811 (16)	...	0.853 (18)	...
Polymer gels ^a	0.702 (21)	...	0.872 (27)	...	0.929 (29)	...

UDas (20)

Pantelis et al, Med Phys. 37, 2369-2379, 2010

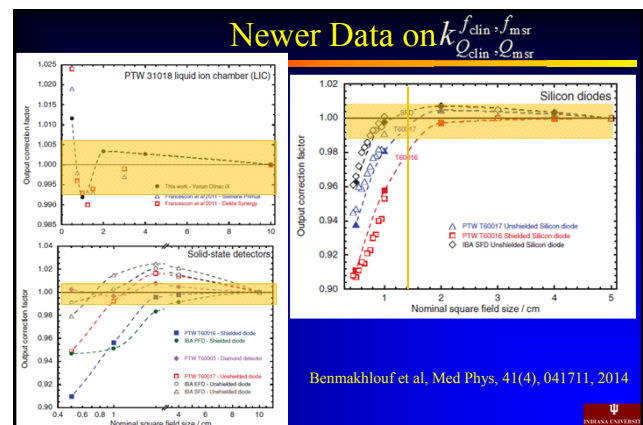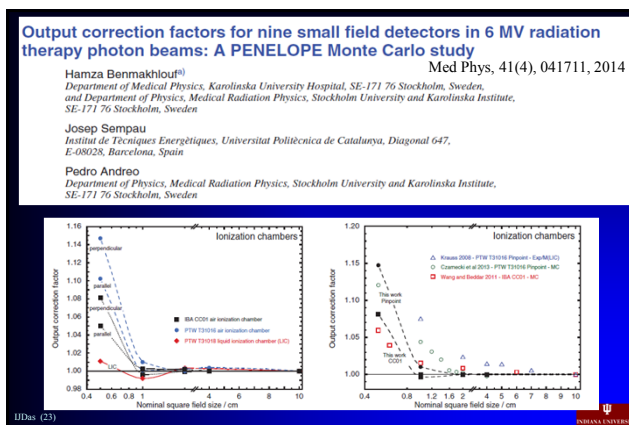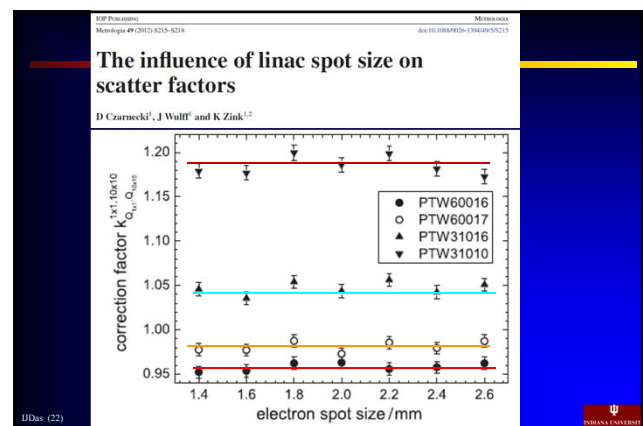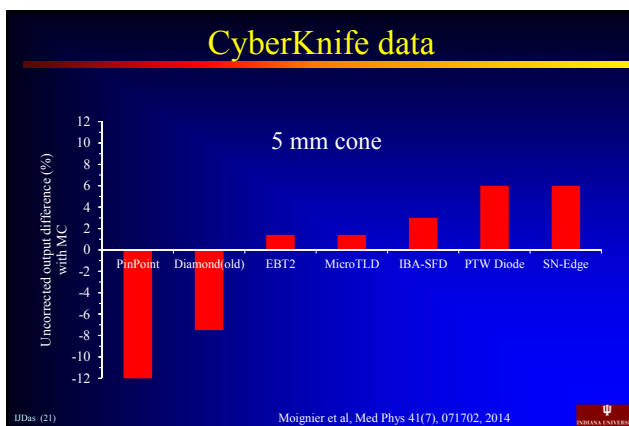

New Published data From IAEA

Detector to detector corrections: A comprehensive experimental study of detector specific correction factors for beam output measurements for small radiotherapy beams

Godfrey Azangwe¹ and Paulina Grochowska
International Atomic Energy Agency, Vienna International Centre, PO Box 100, 1400 Vienna, Austria
Dietmar Geering
Department of Radiation Oncology, Medical University Vienna/KEK Vienna, Währinger Gürtel 18-20, A-1090 Vienna, Austria and Christian Doppler Laboratory for Medical Radiation Research for Radiation Oncology, Medical University Vienna, Vienna, Währinger Gürtel 18-20, A-1090 Vienna, Austria
Joanna Izewska
International Atomic Energy Agency, Vienna International Centre, PO Box 100, 1400 Vienna, Austria
Johannes Henggeler and Wolfgang Lechner
Department of Radiation Oncology, Medical University Vienna/KEK Vienna, Währinger Gürtel 18-20, A-1090 Vienna, Austria and Christian Doppler Laboratory for Medical Radiation Research for Radiation Oncology, Medical University Vienna, Vienna, Währinger Gürtel 18-20, A-1090 Vienna, Austria
Claus E. Andersen, Anders R. Beierholm, and Jakob Helt-Hansen
Center for Nuclear Technologies, Technical University of Denmark, Rise Campus, DK-4000 Roskilde, Denmark
Hideyuki Mizuno and Akifumi Fukumura
National Institute of Radiological Sciences, 4-6-1, Anagawa, Inage-ku, Chiba-shi 263-8555, Japan
Kaori Yajima
Association for Nuclear Technology in Medicine, 7-16, Nishinoharadennomachi, Chama-ku, Tokyo 103-0001, Japan
Clare Gouldstone and Peter Sharpe
National Physical Laboratory, Acoustics and Ionising Radiation Division, Teddington TW11 0EL, United Kingdom
Ahmed Mughalzani
International Atomic Energy Agency, Vienna International Centre, PO Box 100, 1400 Vienna, Austria
Hugo Palmans
National Physical Laboratory, Acoustics and Ionising Radiation Division, Teddington TW11 0EL, United Kingdom and ICR Medical Physics Department, 4-700 Wiener Strasse, Austria

IJDs (25)

072103-11 Med. Phys. 41 (7), July 2014

INDIANA UNIVERSITY

Correction Factors

TABLE V. Detector correction factors (P_{det})_{0.05cm²} and (P_{det})_{0.05cm²} factors shows are ratios of detector ratios relative to the dose rates determined from alanine measurement for each field size ($\frac{P_{det}}{P_{alanine}}$)_{0.05cm²} = ($P_{det}/P_{alanine}$)_{0.05cm²}.

FS [cm]	0.6	0.9	1.2	1.8	2.4	3.0	4.2	10.0
TLD-chips	1.000	...	1.003	1.008	1.004	1.000	1.005	1.010
TLD-micro-chips	0.998	...	1.000	1.001	1.009	1.000	1.001	1.007
IBA SFD-diode	0.995	...	0.998	1.002	1.006	1.000	0.990	0.969
IBA PFD-diode	0.916	...	0.962	0.983	0.999	1.000	1.000	1.001
IBA EFD-diode	0.961	...	0.983	0.992	1.002	1.000	0.997	0.989
PTW 40003Diamond	0.995	...	0.983	0.992	1.002	1.000	0.996	0.995
PTW 60019 microDiamond	0.961	...	0.980	0.990	1.001	1.000	0.999	1.000
RPLD (GDM-302M)	...	...	0.993	0.998	1.000	1.000	0.994	0.997
ASuS-C	0.980	0.982	0.985	0.991	0.999	1.000	...	0.997
Scintillator 1	1.022	1.009	1.000	0.996	1.001	1.000	...	0.992
Scintillator 2	1.028	1.015	1.006	1.000	1.004	1.000	...	0.998
PTW 31013ScintLoon	0.970	...	0.980	0.990	1.000	1.000	0.999	1.005
IBA CCI01	1.000	...	0.993	0.993	1.000	1.000	0.997	0.990
IBA CCI04	1.096	...	1.007	0.998	1.003	1.000	0.997	0.998
IBA CCI13	...	...	1.003	1.008	1.005	1.000	0.996	0.996
Wellhofer ICI0	...	...	1.009	1.005	1.005	1.000	0.996	0.996
PTW 31014 PinPoint	1.034	...	1.007	1.002	1.000	1.000	0.998	1.002
PTW 31016 PinPoint 3D	1.078	...	1.013	1.000	1.001	1.000	0.998	0.999
PTW 31013 ScintLoon ^h	...	...	1.027	1.002	1.004	1.000	0.996	0.997
PTW 31013 ScintLoon ^h	...	...	1.013	1.000	1.000	1.000	0.992	0.991


^hThis chamber was included in the table for completeness but it is not recommended to use for small field dosimetry in fields smaller than 2.0 × 2.0 cm² because the volume averaging effect is unacceptably high.
ⁱFor these ionization chambers, corrections for the smallest field were unacceptably high (>20%) for field sizes smaller than 1 × 1 cm² and therefore were excluded from Table V.

IJDs (26)

INDIANA UNIVERSITY

Variation of $k_{Q_{50,50}}$ for the small-field dosimetric parameters percentage depth dose, tissue-maximum ratio, and off-axis ratio

Paolo Francescon¹
Department of Radiation Oncology, Ospedale Di Vienna, Viale Rodolfo, Vienna 30100, Italy
Sam Beedjar
Department of Radiation Physics, The University of Texas MD Anderson Cancer Center, Houston, Texas 77030
Nirina Satariano
Department of Radiation Oncology, Ospedale Di Vienna, Viale Rodolfo, Vienna 30100, Italy
Indra J. Das
Department of Radiation Oncology, Indiana University School of Medicine, Indianapolis, Indiana 46202

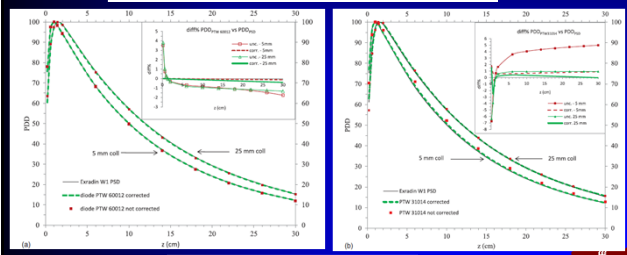


IJDs (27)

Med. Phys. 41 (10), October 2014 0094-2405/2014/41(10)/101708

INDIANA UNIVERSITY

Correction in Profile (OAR)

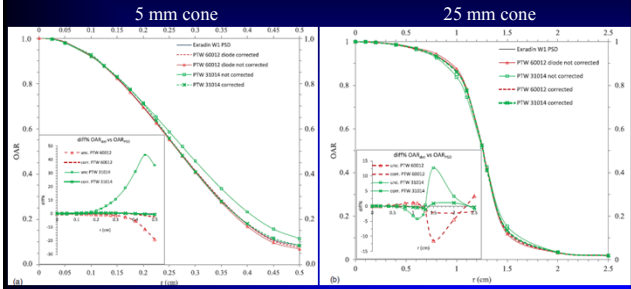


IJDs (28)

Francescon et al, Med Phys, 41(10), 101708, 2014

INDIANA UNIVERSITY

Depth Dose & Source Size

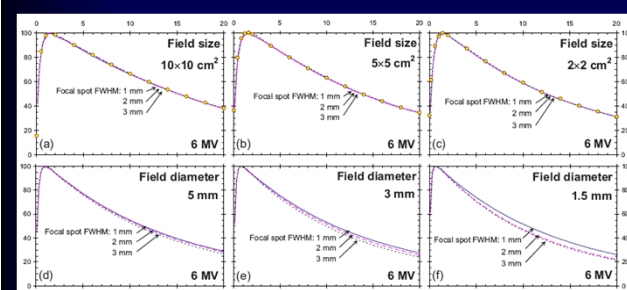


IJDs (29)

Sham et al, Med Phys, 35, 3317-3330, 2008

INDIANA UNIVERSITY

Good News with Modern Microdetectors

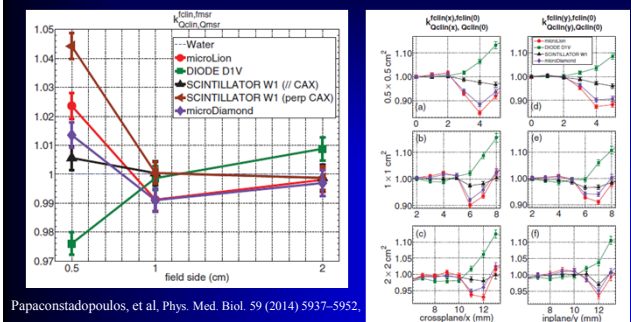

Papaconstadopoulos, et al, Phys. Med. Biol. 59 (2014) 5937-5952,

IJDs (30)

INDIANA UNIVERSITY

