UCLA

Ke Sheng, Ph.D., DABR
Professor of Radiation Oncology
University of California, Los Angeles

MR SIMULATION FOR RADIOTHERAPY

The need for MRI in radiotherapy

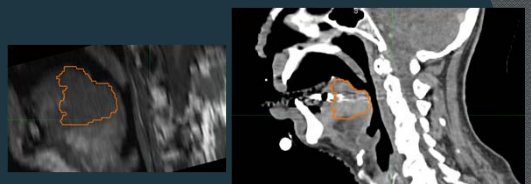

T1 FSE

CT

Tumor and normal tissues in brain, breast, head and neck, liver, prostate, cervix, rectal etc. are much better visualized in MRI than CT

UCLA

Multiparametric MRI reflects a more complete picture of the tumor biology

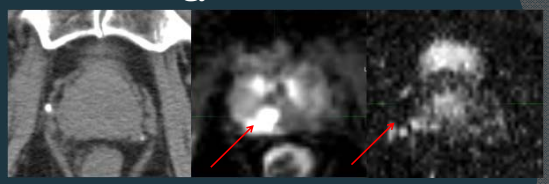

CT DCE MRI ADC MRI

MRI is typically used to detect Intraprostatic lesions

UCLA

Simultaneous integrated boost of the intraprostatic lesions



Onal et al. Br J Radiol. 2014 87(1034):20130617.

UCLA

MR guided radiation therapy

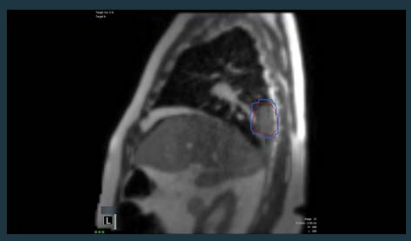

Dynamic MRI images recorded during ViewRay treatment. MRI guided radiotherapy provides high quality internal anatomy images during the treatment

UCLA

MR geometrical distortions

Compared to CT, MR images have an intricate geometric distortion problem that is caused by:

- B0 inhomogeneity
  - Can be corrected by shimming
- Susceptibility (tissue air/bone interface)
- Gradient nonlinearity
  - Contribute most to observed distortion
- Chemical shift
  - Relatively small

The distortion if uncorrected may be cause segmentation and dose calculation errors in radiotherapy relying on MR simulation.

UCLA

Understanding the distortion correction

Siemens Sonata 1.5 T

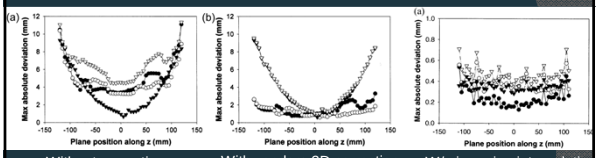

Without correction | With vendors 2D correction | W/ piecewise interpolatio

Wang et al. Magnetic Resonance Imaging 22(9), 2004, PP 1211–1232

Distortion increase with increasing distance to the isocenter
Vendors' correction is typically effective with limitations
xy correction does little to correct the distortion along the z direction

UCLA

MR image distortions using a pelvic phantom and deformable registration

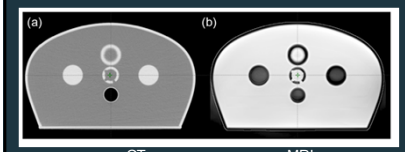

CT MRI



For Siemens Skyra 3T scanner, vendor's 2D and 3D distortion correction methods reduce the error from 7.5 mm to 2.6 and 1.7 mm respectively

Sun et al. Phys. Med. Biol. **60** (2015) 3097–3109

UCLA

Question 1: MRI geometrical distortion is caused by?

20% (a). B0 field inhomogeneity
20% (b). Susceptibility artifacts
20% (c). Chemical shift
20% (d). Gradient nonlinearity
20% (e). All the above

UCLA

Answer to question 1

(e). All the above

Reference: Wang et al. Magnetic Resonance Imaging 22(9), 2004, PP 1211–1232

UCLA

MRI simulation for RTP: fusion



Devic S. Medical Physics 39, 6701 (2012)

UCLA

MR-CT registration

Rigid/manual registration
- Example: Brain, head and neck

Affine registration
- Example: Head and neck

Deformable registration
- Example: Abdominal and pelvis

UCLA

Cranial rigid registration

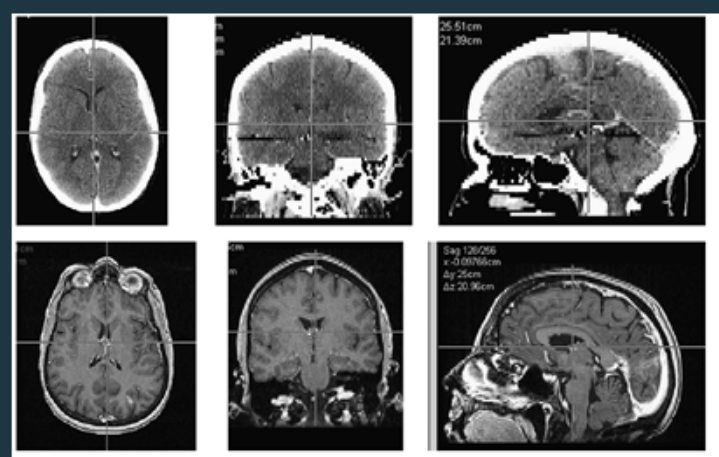

45 institutions and 11 software registered a set of CT and MR with known ground truth based on BRW (Brown-Roberts-Wells) stereotactic head frame

Ulin K et al Int J Radiat Oncol Biol Phys. 2010 Aug 1;77(5):1584-9

UCLA

13

Cranial rigid registration

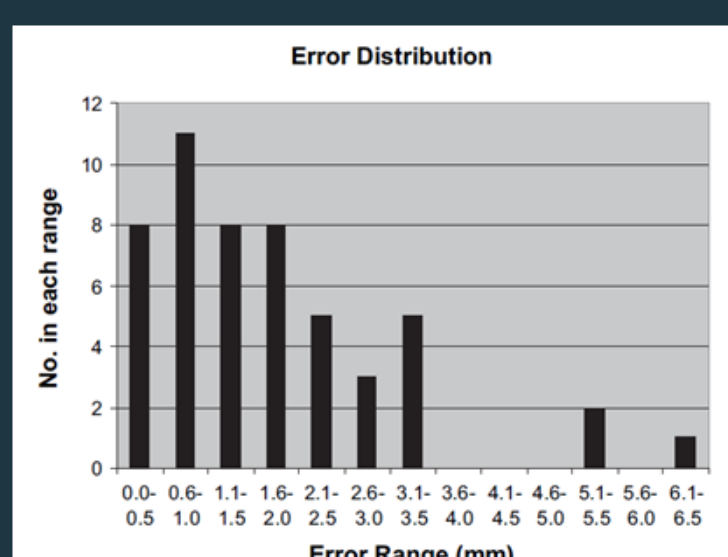

Ulin K et al Int J Radiat Oncol Biol Phys. 2010;77(5):1584-9

UCLA

14

MR-CT registration

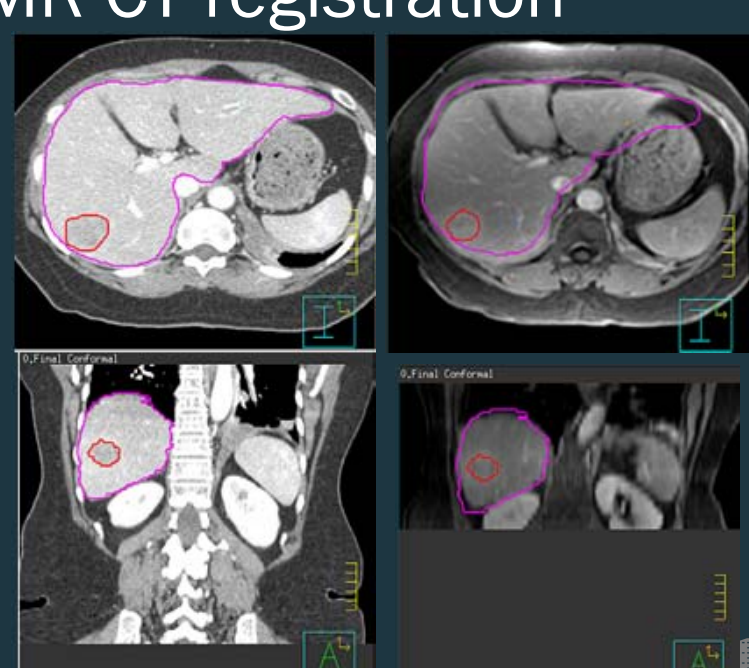

The mean absolute error for the liver ranged from 1.1 to 5.0 mm,

Brock KK. Int. J. Radiation Oncology Biol. Phys., 76(2), pp. 583–596

15

MR CT registration of the prostate

CT B-spline warped MR Adaptive FEM

Average prostate centroid distance 3.7 mm using commercial B-spline registration

Zhong et al. Phys. Med. Biol. 60 (2015) 2837–2851

UCLA

MRI only simulation

- Avoid the uncertainties from MR-CT registration
- Reduce patient exposure to imaging doses
- For MR guided radiotherapy, the MR simulation provides more native imaging format for registration (avoid CT-MR registration during IMRT)

Challenges

- Need electron density for dose calculation and CT IGRT
- Not straightforward to generate DRR
- Compromise between limited FOV and high resolution
- Low throughput

UCLA

DRR from pseudo MRI

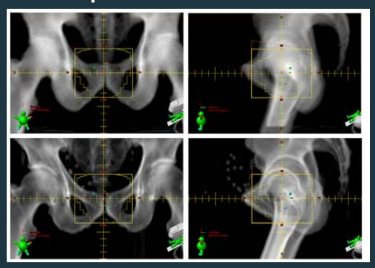

Manual, semi-automated and automated bone segmentation was used to create pelvic bony anatomies from MR and then DRR

Chen L et al. IJROBP 68(3), 2007, pp 905–911

Dowling JA et al., IJROBP 83 (1), 2012, pp e5–e11

MRI only simulation



Creating bony anatomies for the head and neck region is more difficult due to abutting airways.

Manual contouring of all airways was used to create air mask and then subtract from the automated MR bone segmentation

Yu H et al. IJROBP 89(3), 2014, Pages 649–657

UCLA

DRR from MRI

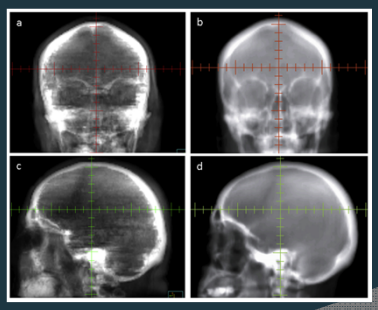

Yu H et al. IJROBP 89(3), 2014, Pages 649–657

UCLA

Ultra-short TE MRI

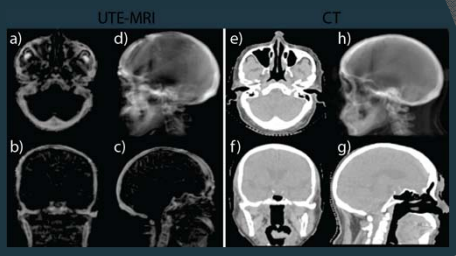

T2 relaxation time of cortical bones~1 ms vs 250 ms in tissue

Ultra-short TE MR has been used to image the bones directly

Yang Y et al. Under review

UCLA

Electron density estimation for MRI

- Direct segmentation
  - Bulk density assignment
- Atlas based method
  - Generate average MR/CT data set with individual organ labeling
- Classification-based method
  - Based on image texture analysis and learning

Require a priori CT-MR registration

UCLA

Impact of electron density estimation for prostate IMRT

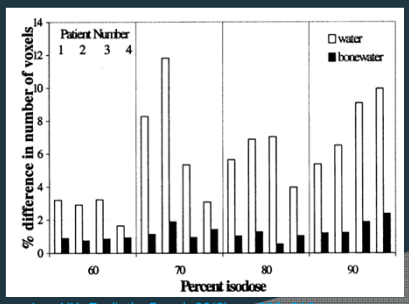

Lee YK, Radioth. Oncol. 66(2), pp 203-216

Residual error <2%

Impact of electron density estimation for head and neck IMRT

head and neck IMRT

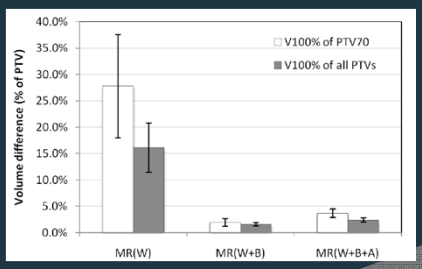

Bones accounts for the majority of density heterogeneity effects

Residual error ~2%

Chin AL, et al., JACMP, Vol 15, No 5, 2014

Other heterogeneous density objects

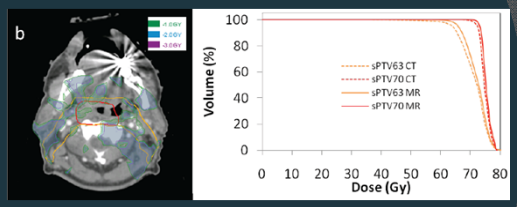

Assigning cortical bone density to the implant results in 4% dose calculation error.
Correction of such errors may require laborious manual segmentation of the implant.

Chin AL et al. JACMP Vol 15, No 5 (2014)

25

Question 2: Compared to CT, what is the expected dosimetric difference using MR for planning after density correction?

20% (a). 0.5%
20% (b). 2%
20% (c). 8%
20% (d). 12%
20% (e). 18%

UCLA

26

Answer to question 2

(b). 2%

- References: Brock KK. Int. J. Radiation Oncology Biol. Phys., 76(2), pp. 583–596
- Zhong et al. Phys. Med. Biol. 60 (2015) 2837–2851

UCLA

27

Summary

- MRI is becoming increasingly important in radiotherapy
- MRI geometrical distortion can be manageable using the vendors' tool but it needs to be rigorously QA'd for both the specific machine and the process.
- MRI-CT registration is challenging and error prone, particularly deformable registration.
- Multiple methods are available to assign electron density to MRI for dose calculation and generation of DRR.
- The process to assign electron density can involve manual segmentation that is labor intensive.
- Bone (teeth) density contributes to the majority of density heterogeneity effects.